128/227 X 604/96

Colonic Frame
Scale ¼" = 1"

Vacuum Break

Flow Control Valve

Glass Tube

Thermometer

Plug

Thermostatic Control

Inflow to Patient

Outflow From Patient

Plug

Move

Plug

Move

Belong in Center

Plug

air vent

Mixing Tank

Hot W

Cold W

A

Overflow to sewer

Air Break

Vacuum Break

Flow

When pressure is released disk drops to lower seat providing air break and preventing back syphonage of water in fixture to supply line.

supply

Aspirator

AIV

City Pressure

Regulate flow to patient.

After passing thru. aspirator and being mixed with air.

Over that the patient cannot accommodate This affords a release so there can be no back pressure.

Over flow so there cannot be over a 3 oz. maximum pressure at any time to the patient.

Air vent line to break any vacuum that might be created.

PATENT OFFICE
JUN 17 1941
DIV. 55

Vacuum Break

Flow Control Valve

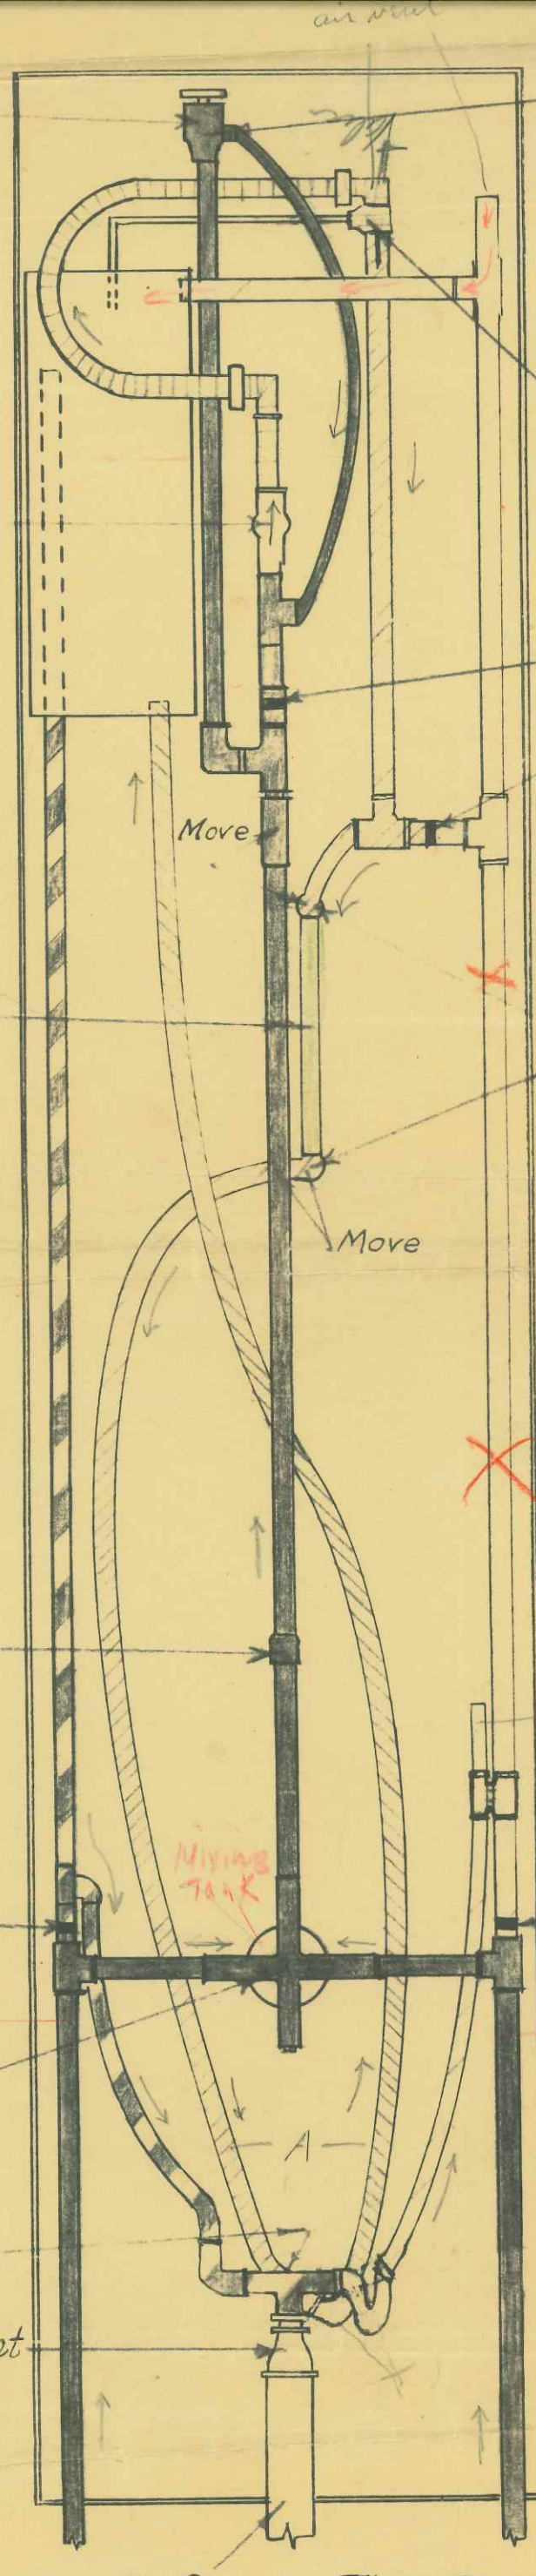

When pressure is released disk drops to lower seat providing air break and preventing back syphonage of water in fixture to supply line.

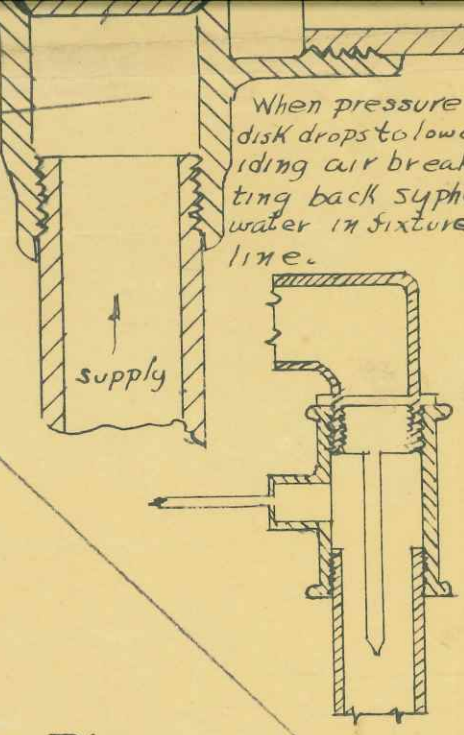

Aspirator

A IV

Plug

Plug

Glass Tube

Belong in Center

Thermometer

Plug

Plug

Thermostatic Control

Inflow to Patient

Outflow From Patient

To Sewer Thru Trap

City Pressure

Regulate flow to patient.

After passing thru. aspirator and being mixed with air.

Over that the patient cannot accommodate This affords a release so there can be no back pressure.

Over flow so there cannot be over a 3 oz. maximum pressure at any time to the patient.

Air vent line to break any vacuum that might be created.

PATENT OFFICE

JUN 17 1941

DIV. 55

Dan Coombs
K. C. Mo.

J.V. Cowles 4-22-39